

Pittsburg State University

Pittsburg State University Digital Commons

Posters

2019 Research Colloquium

4-1-2019

Agreement Study Between the ParvoMedics TrueOne 2400 and Vacu-Med Vista MINI-CPX Metabolic Measurement System

Mohan D. Perumal

Pittsburg State University

Allison M. Barry

Pittsburg State University

Michael Carper

Pittsburg State University

Derek A. Crawford

Pittsburg State University

Follow this and additional works at: https://digitalcommons.pittstate.edu/posters_2019



Part of the [Community Health and Preventive Medicine Commons](#)

Recommended Citation

Perumal, Mohan D.; Barry, Allison M.; Carper, Michael; and Crawford, Derek A., "Agreement Study Between the ParvoMedics TrueOne 2400 and Vacu-Med Vista MINI-CPX Metabolic Measurement System" (2019). *Posters*. 50.

https://digitalcommons.pittstate.edu/posters_2019/50

This Article is brought to you for free and open access by the 2019 Research Colloquium at Pittsburg State University Digital Commons. It has been accepted for inclusion in Posters by an authorized administrator of Pittsburg State University Digital Commons. For more information, please contact digitalcommons@pittstate.edu.

Introduction

- Aerobic capacity ($\text{VO}_{2\text{MAX}}$) predicts both athletic performance and health status. Many tools are available to assess VO2 MAX ranging in both cost and accuracy.
- Understanding limitations of less expensive tools, likely found in settings such as health clinics or sports performance facilities, will help practitioners in developing accurate exercise prescriptions for their respective populations.

Purpose

To evaluate agreement lower cost $\text{VO}_{2\text{MAX}}$ assessment tool (Vacu-Med Vista MINI-CPX) to the industry “gold standard” (ParvoMedics TrueOne 2400).

Methods

- Thirty-one participants (22.5 ± 3.5 years; BMI 24.9 ± 2.3 ; 51% female) completed two sessions of maximal $\text{VO}_{2\text{MAX}}$ assessment using the Bruce Protocol graded treadmill exercise test.
- The first session of assessment utilized the “gold-standard” unit (TrueOne 2400, ParvoMedics, Inc., Murray, UT)..
-). 24-48 hours later the second unit (Vista Mini-CPX, Vacu-Med, Inc., Ventura, CA) was used to assess $\text{VO}_{2\text{MAX}}$ again.

Agreement Study between the ParvoMedics TrueOne 2400 and Vacu-Med Vista MINI-CPX Metabolic Measurement System

Mohan D. Perumal¹, Allison M. Barry¹ , Michael Carper¹, Derek A. Crawford¹

¹Health, Human Performance, and Recreation; Pittsburg State University; Pittsburg, Kansas

Statistical Analysis

- A Bland-Altman analyses was used to evaluate both potential bias and agreement for between the two assessment tools.

Results

- The CPX unit significantly overestimated $\text{VO}_{2\text{MAX}}$ compared to the TrueOne (Bias = 10.67 ± 5.87 ml/kg/min, LoA = -0.83, 22.18; t = 1.96, $p < .001$).
- However, the CPX unit demonstrates good reliability as 93.5% (29/31 participants) of values fell within the 95% LoA.
- Further, values above 46.5 ml/kg/min tend to be greater than the mean bias while those below tend to be lower than the mean bias ($r = .605$, $F = 16.80$, $p < .001$).

TABLE 1. Participant Characteristics

| | Age (year) | Sex | BMI | Fat Mass (kg) | Fat Free Mass (kg) |
|------------------------|----------------------|--------------------|---------------------|----------------------|-----------------------|
| Participants (n=31) | 22.939 ± 4.24 | M=51.5% F=48.5% | 24.96 ± 4.11 | 22.77 ± 11.08 | 53.65 ± 13.31 |

TABLE 2. Regression Statistics

| Regression Statistics | |
|-----------------------|-------------|
| Multiple R | 0.605681505 |
| R Square | 0.366850085 |
| Adjusted R Square | 0.345017329 |
| Standard Error | 4.752696697 |
| Observations | 31 |

TABLE 3. ANOVA

| ANOVA | df | SS | MS | F | Significance F |
|------------|----|-------------|----------|----------|----------------|
| Regression | 1 | 379.5423732 | 379.5424 | 16.80274 | 0.000305471 |
| Residual | 29 | 655.055651 | 22.58813 | | |
| Total | 30 | 1034.598024 | | | |

Results

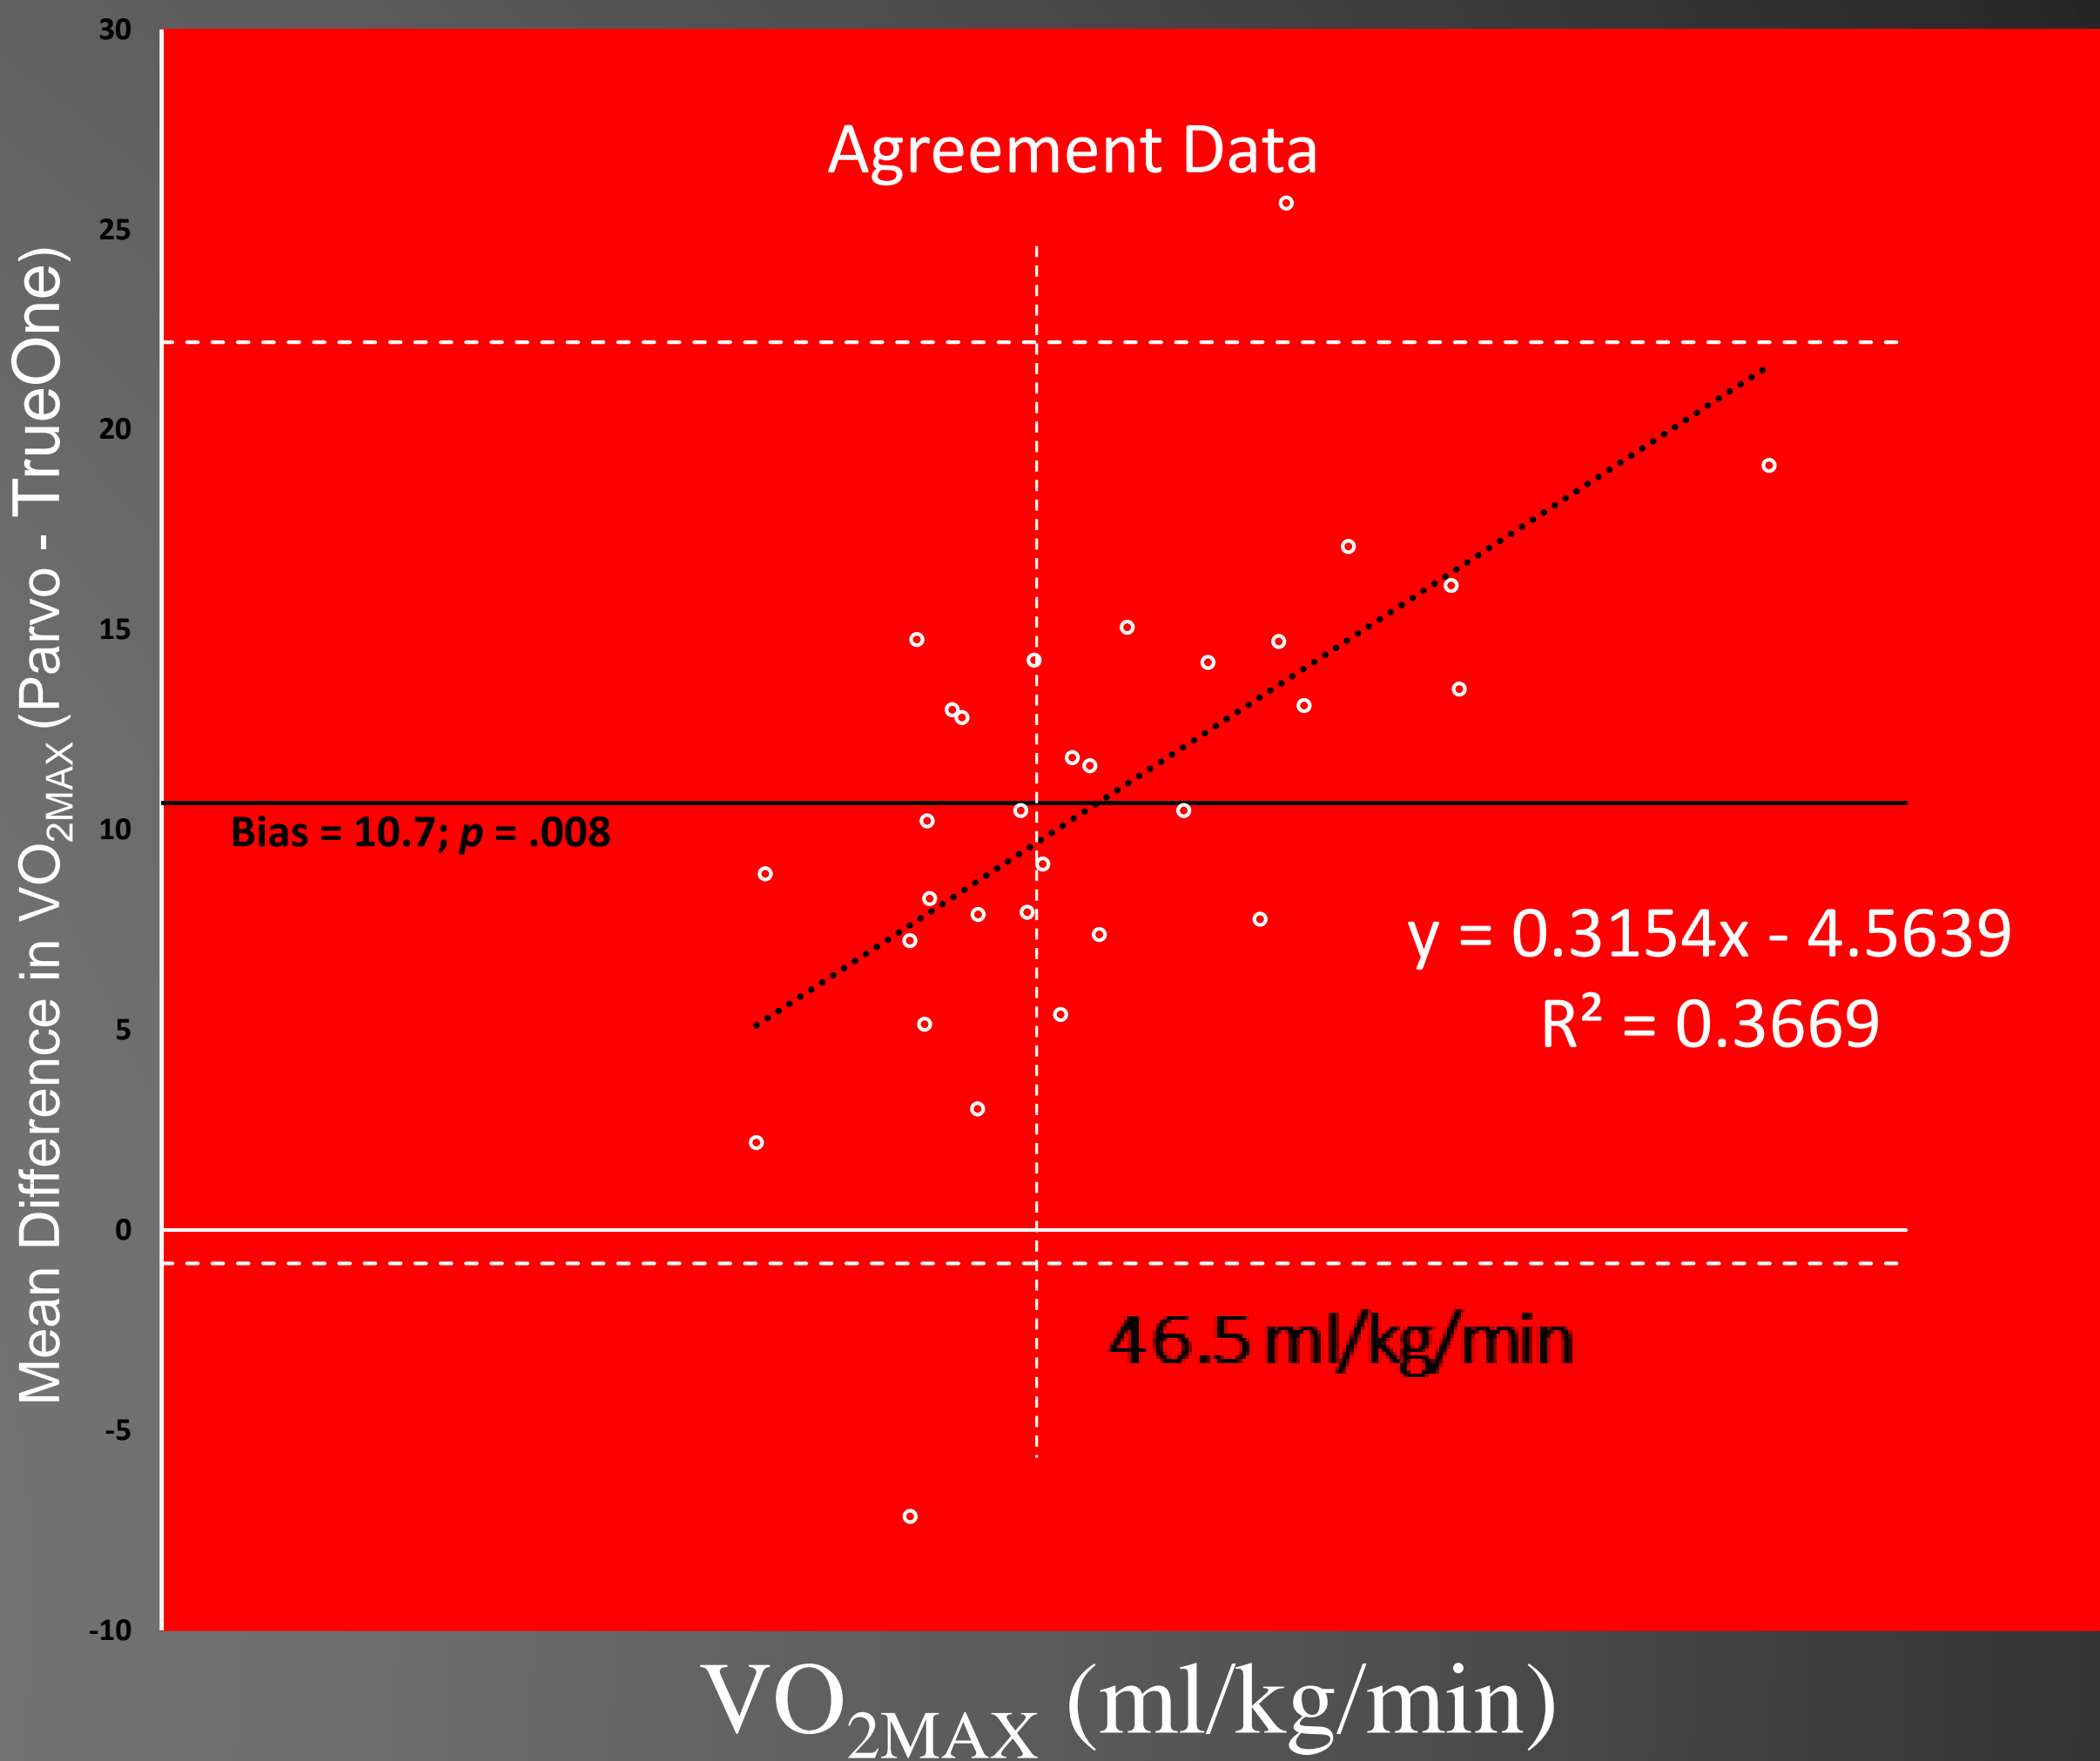


Figure 1. Agreement Data

Conclusion

- The CPX unit demonstrates good reliability yet a significant overestimation of aerobic capacity.
- The CPX is a tool that can be used for individuals that are less trained, more average individuals.
- For clinical populations the CPX is a good tool for assessing cardiopulmonary fitness.
- For trained athletes and individual that work out regularly, should use the Parvo Medics to assess aerobic capacity.

References

1. Accuracy and reliability of the ParvoMedics TrueOne 2400 and MedGraphics VO2000 metabolic systems.
https://scholar.google.com/scholar?hl=en&as_sdt=0%2C5&q=validation+for+ParvoMedics+TrueOne+2400&btnG=#d=gs_cit&u=%2Fscholar%3Fq%3Dinfo%3A1aholKfNSEoJ%3Ascholar.google.com%2F%26output%3Dcite%26scirp%3D0%26hl%3Den